

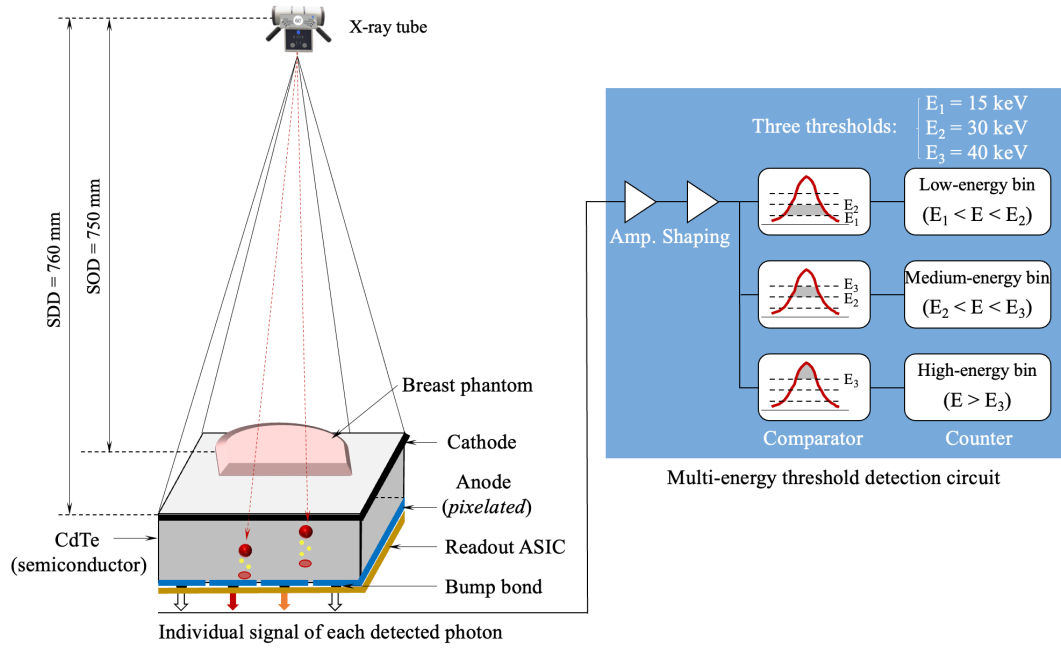


Figure 1. Schematic diagram of the CdTe-based photon-counting detector system for breast phantom imaging with three energy thresholds

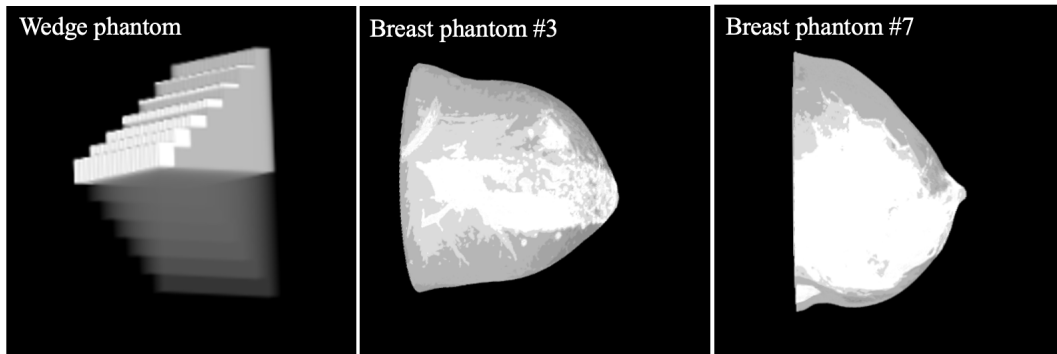


Figure 2. Wedge phantom and two examples (#3 and #7) from the set of nine breast phantoms.

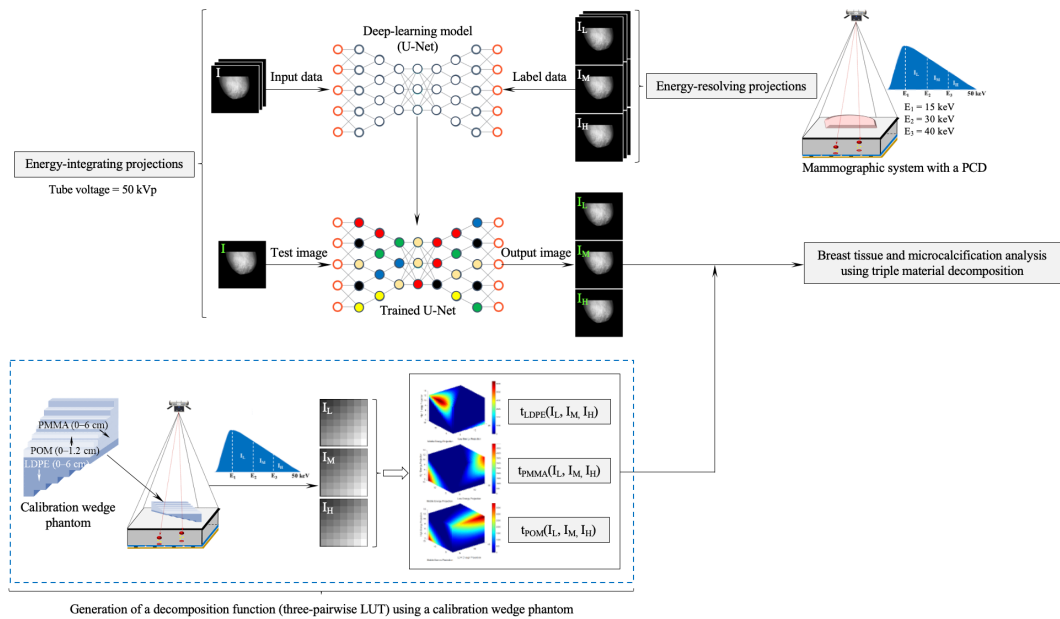


Figure 3. Workflow of PCD-like projection generation and triple material decomposition for breast analysis.